




6/23

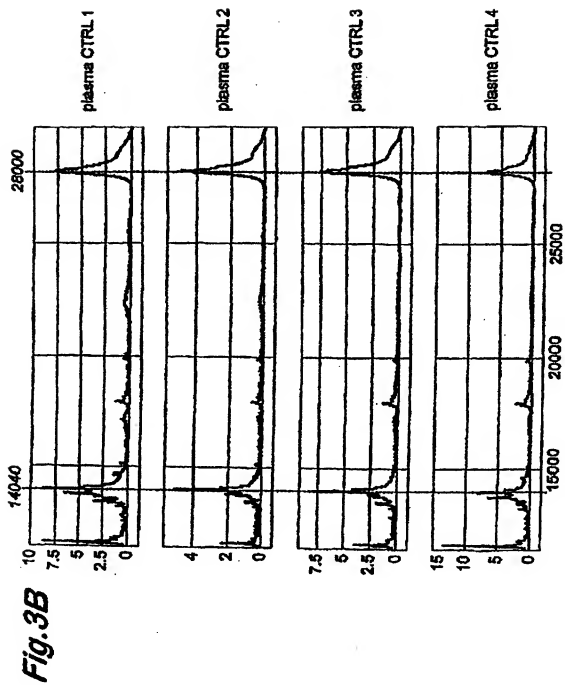


7/23

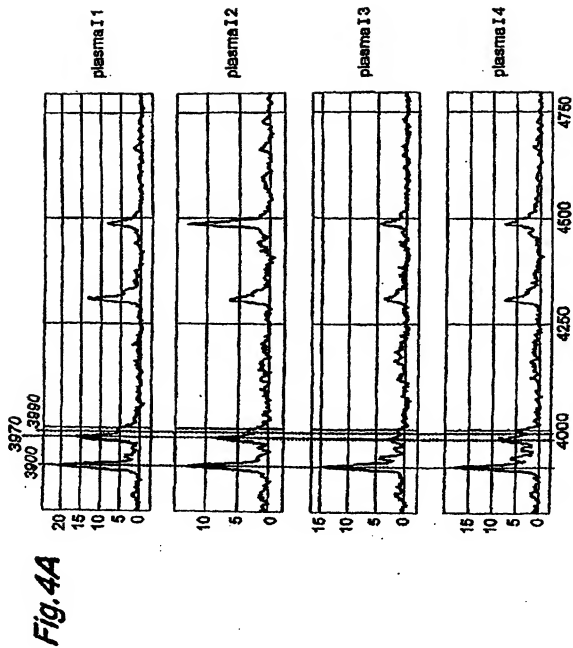


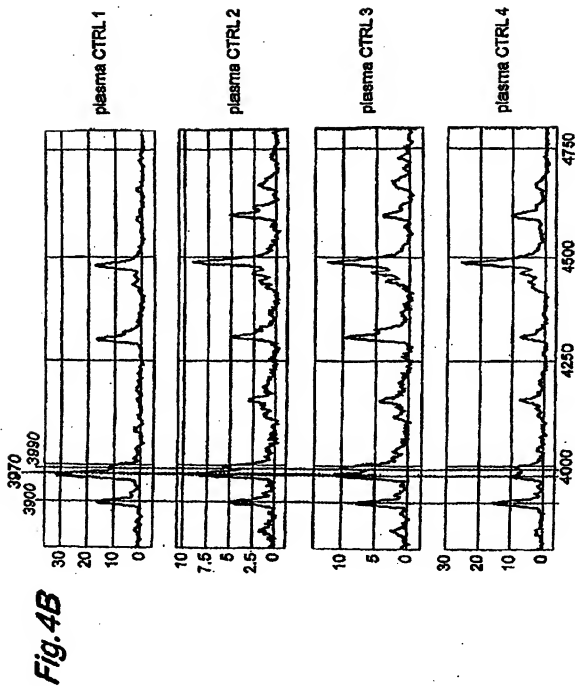



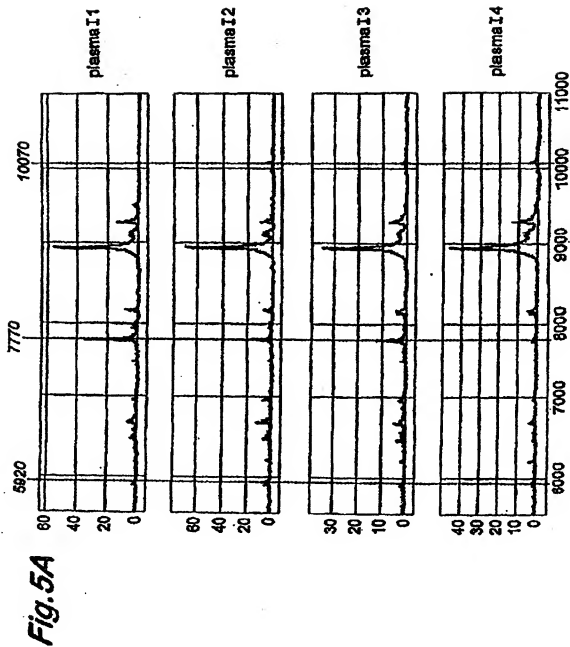

10/23

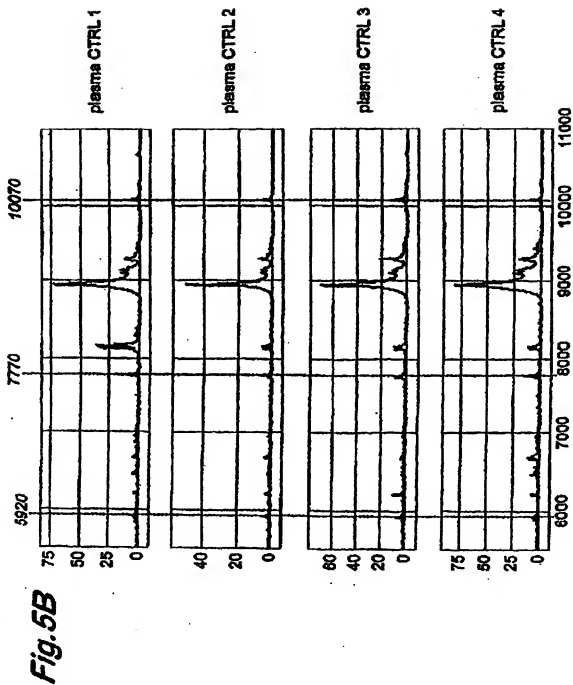

11/23

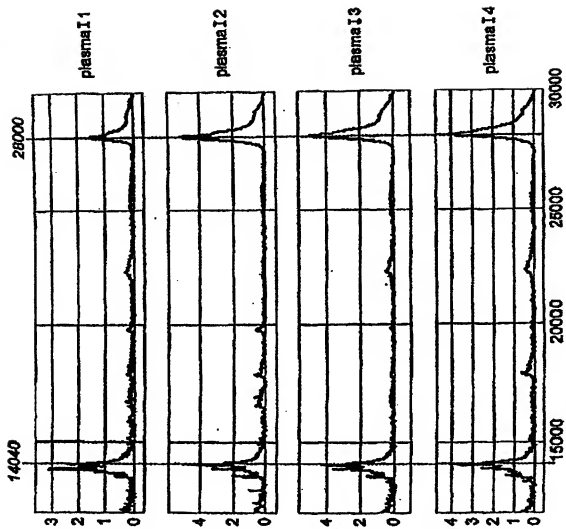


Fig. 6A

12/23

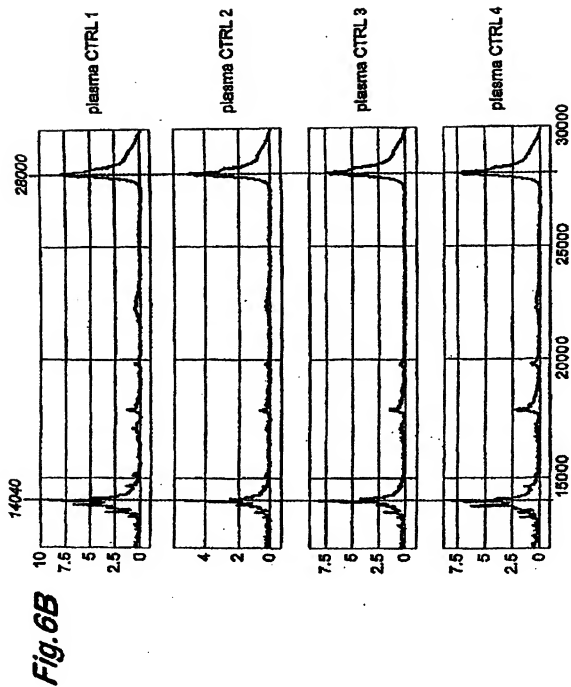


Fig. 7A

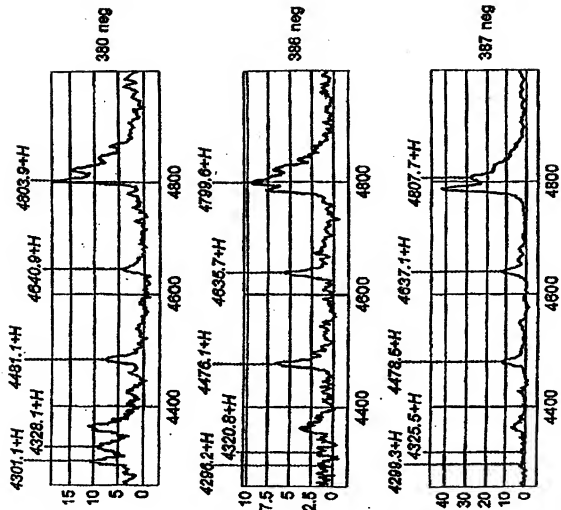
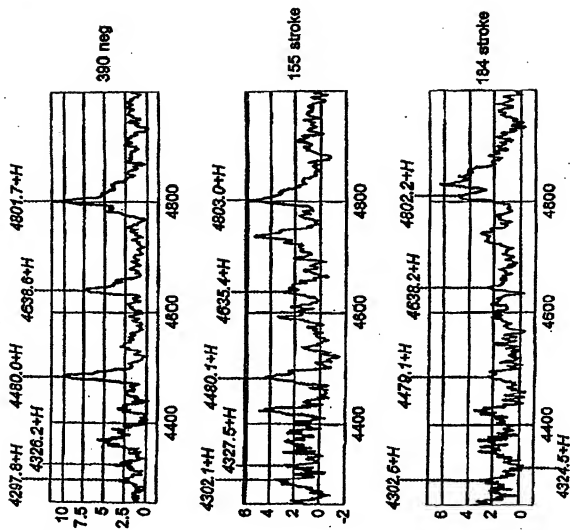
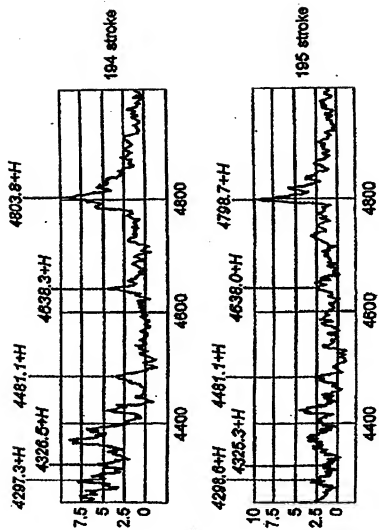
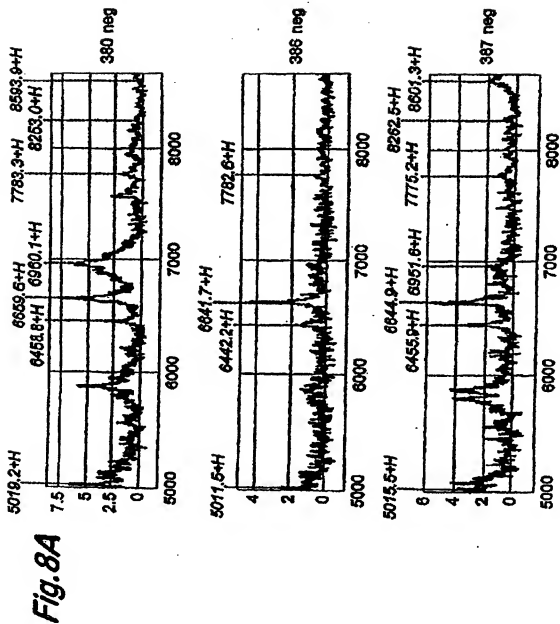



Fig. 7B









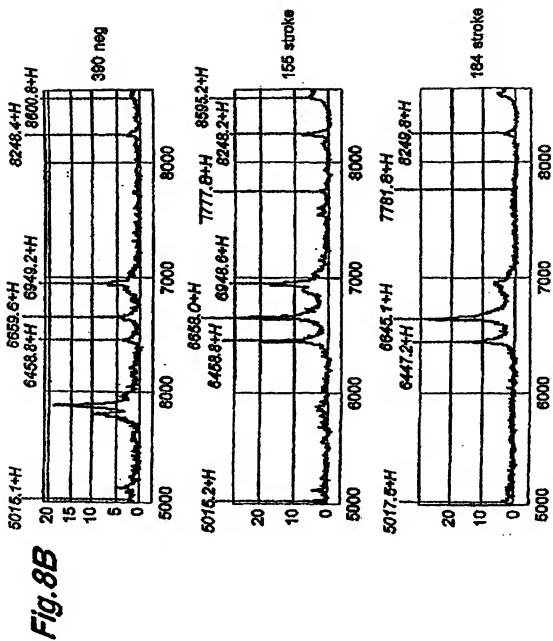

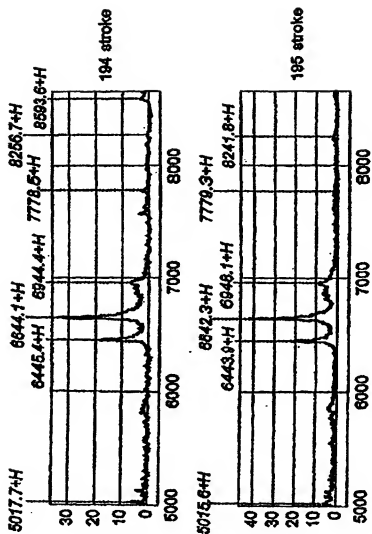


Fig. 9A

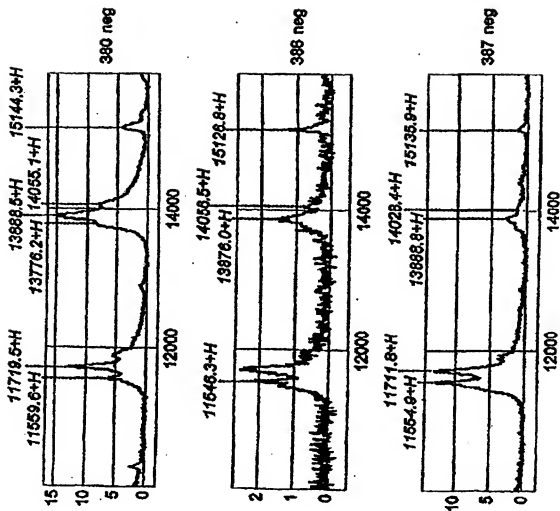
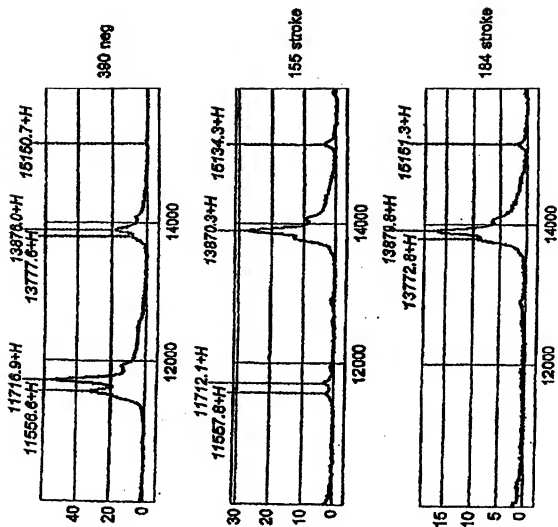


Fig. 9B




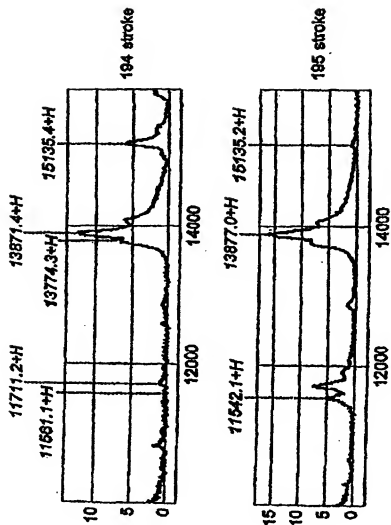


Fig.9C

Figure 10. Determination of ApoC-III level in 14 haemorrhagic and 13 ischaemic stroke plasma samples compared to 30 negative controls using Daiichi tests (Cobas Mira plus automate)

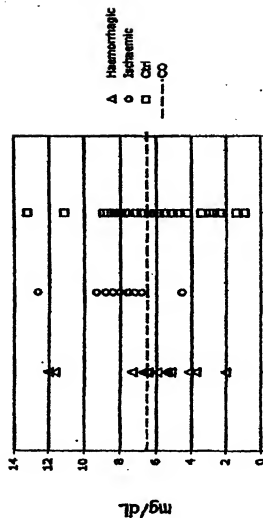

	P (student test)	Sensitivity	Specificity
I vs H	0.0342	92.3 %	71.42 %
I vs Ctrl	0.025	92.3 %	50 %
H vs Ctrl	0.4682	-	-

Fig. 11

